

## Scope of Accreditation For Brechtbuhler Scales, Inc.

1414 Scale Street SW  
Canton, OH 44706  
Jim Kullman  
330-458-3062

In recognition of a successful assessment to ISO/IEC 17025:2005, accreditation is granted to **Brechtbuhler Scales, Inc.** to perform the following **Calibrations**:

Accreditation granted through: **May 7, 2013**

### Calibration


#### Mass – Scale and Balances

Calibration Parameter/Equipment <sup>1</sup>	Range	Calibration and Measurement Capability(+/-) <sup>2</sup>	Remarks
Weighing Systems			ASTM E617 Class I Weights and NIST Handbook 44 utilized for the calibration of the weighing systems
0.0001 g resolution	(0 to 320) g	0.7 mg	
0.001 g resolution	(0 to 1200) g	2.6 mg	
0.01 g resolution	(0 to 4100) g	13.8 mg	ASTM E617 Class II Weights and NIST Handbook 44 utilized for the calibration of the weighing systems
0.01 g resolution	(0 to 100) g	5.8 mg	
0.02 g resolution	(0 to 200) g	13.5 mg	
0.1 g resolution	(0 to 5) kg	0.06 g	NIST 105 Class F Weights and NIST Handbook 44 utilized for the calibration of the weighing systems
0.001 lb resolution	(0 to 1) lb	0.0006 lb	
0.001 g resolution	(0 to 30) kg	0.002 kg	
0.01 lb resolution	(0 to 10) lb	0.006 lb	
0.1 g resolution	(0 to 10) kg	0.08 g	

<b>Calibration Parameter/Equipment <sup>1</sup></b>	<b>Range</b>	<b>Calibration and Measurement Capability(+/-) <sup>2</sup></b>	<b>Remarks</b>
0.1 lb resolution	(0 to 1000) lb	0.08 lb	NIST 105 Class F Weights and NIST Handbook 44 utilized for the calibration of the weighing systems
0.5 lb resolution	(0 to 5000) lb	0.4 lb	
1 lb resolution	(0 to 10 000) lb	0.6 lb	
20 lb resolution	(0 to 200 000) lb	16 lb	

Notes:

- 1) Laboratory offers calibration services at the laboratory's own facilities and at the client or other agreed upon facilities.
- 2) Calibration and Measurement Capability represents expanded uncertainties at approximately a 95% confidence level using a coverage factor of k=2.

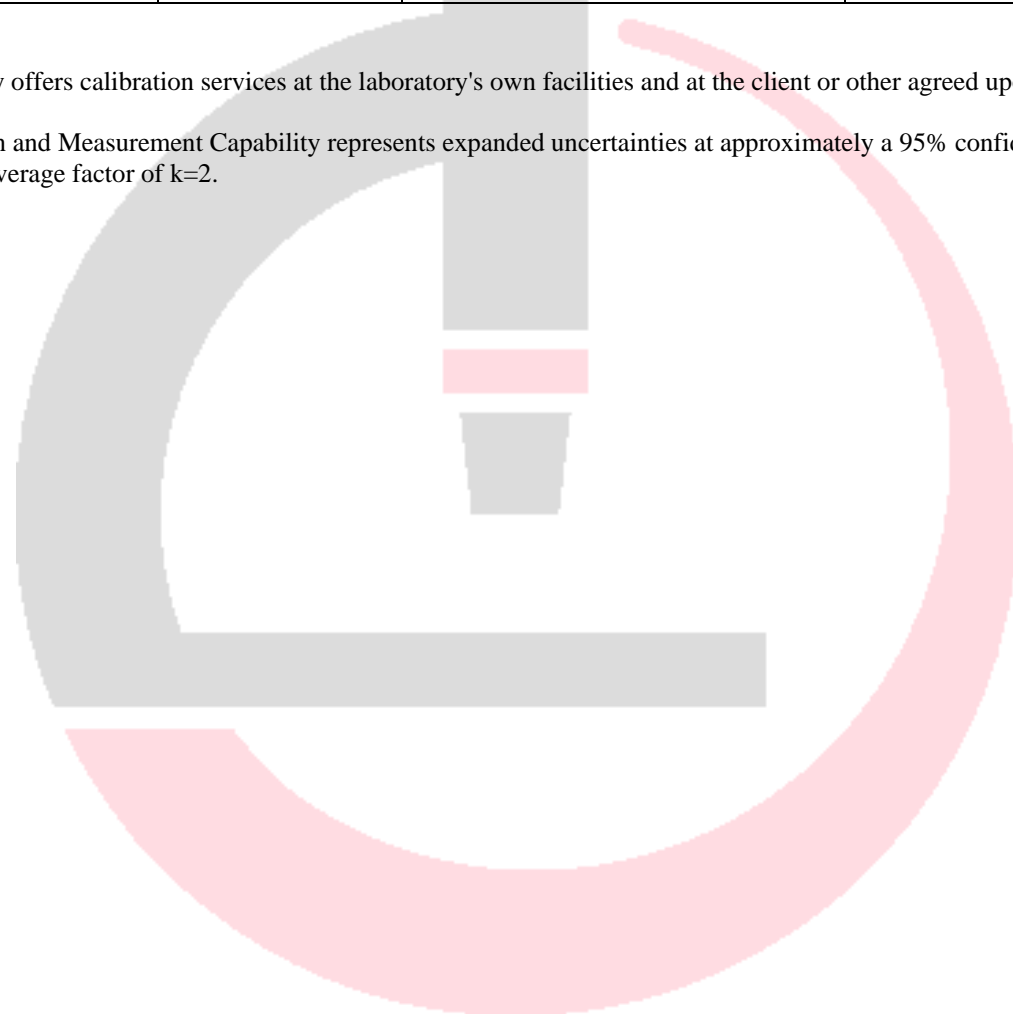

Approved by:   
 R. Douglas Leonard  
 Chief Technical Officer

Date: September 2, 2010

Re-issued: 4/21/10      Revised: 8/20/10      Revised: 9/2/10